

BATINGA ANIMAL MEDICAL CENTER

Nucleic Acid Test Report

Pet Name: MIZZI  
Gender: Female  
Sample No.:  
Test Item: FPI(FPV)

Owner Tel.:  
Species: Feline  
Test Time: 2025-10-15 09:05

Owner Name: EDUARTE  
Pet Age:  
Case No.:

Test Results

Test Item	CT	Reference	Result
FPV	11.5	>36.0 Or NoCt	Positive(+)
IC	20.8	>38.0 Or NoCt	Positive(+)

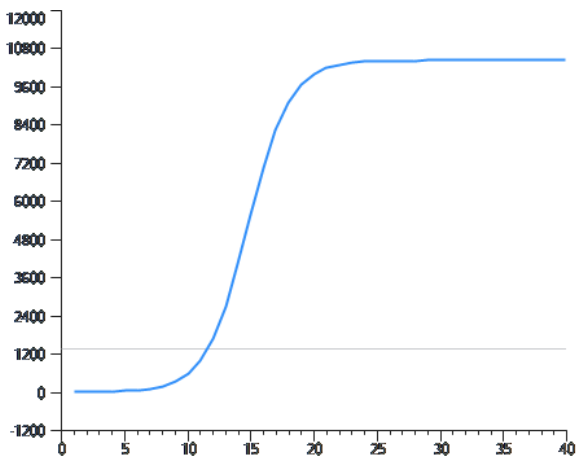


Fig. 1 FPV

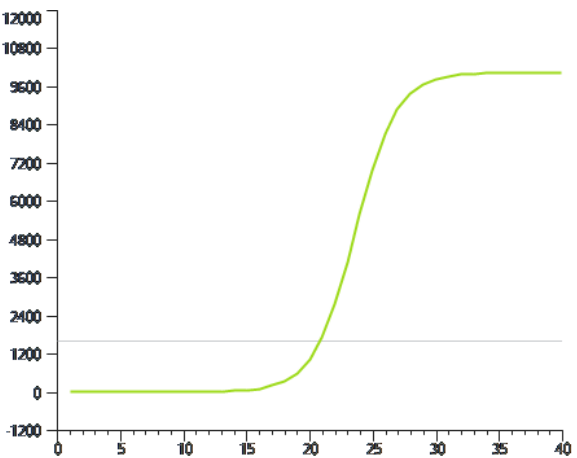


Fig. 2 IC

Result Interpretation:

- Positive Result (+): The current test sample contains the target substance (pathogen or internal control);
  - Negative Result (-): The target substance (pathogen or internal standard) in the current test sample is either below the detection limit or absent;
  - CT > Ref. Range, suggests infection window or recovery phase. Clinical correlation required. Recommend retesting within 24-48 hours to monitor CT dynamics;
  - CT Number Reference Interval: Reference interval used to distinguish the presence or absence of the target substance based on CT numbers.If CT > 30, the viral load is low, and the risk of transmission is low, indicating that the animal may be asymptomatic or in a subclinical state.
- Note: The test results are only valid for the samples submitted this time and are for clinical reference only.

Testing Physician:

Chief Physician:

Hospital Tel.: 09061211260

Report Date: 2025-10-15

Hospital Addc: SM CITY CDO UPTOWN, MASTERSONS AVE., CARMEN, CAGAYAN DE ORO

