

BATINGA ANIMAL MEDICAL CENTER

Nucleic Acid Test Report



Pet Name: TABY
Gender: Female
Sample No.:
Test Item: CPI(CPV)

Owner Tel.:
Species: Canine
Test Time: 2025-10-18 11:52

Owner Name: ESTEVEZ
Pet Age:
Case No.:

Test Results

Test Item	CT	Reference	Result
CPV	15.0	>36.0 Or NoCt	Positive(+)
IC	20.0	>38.0 Or NoCt	Positive(+)

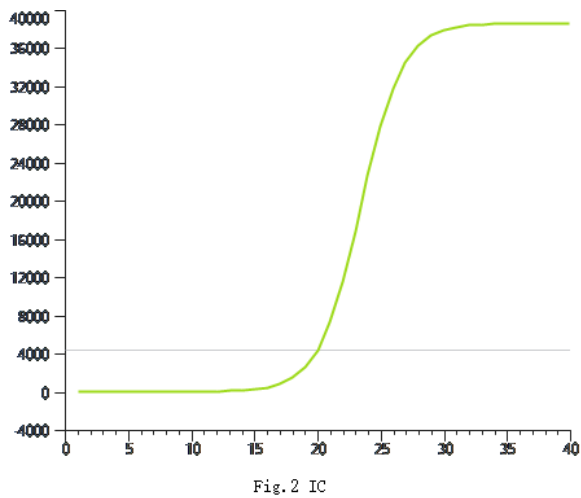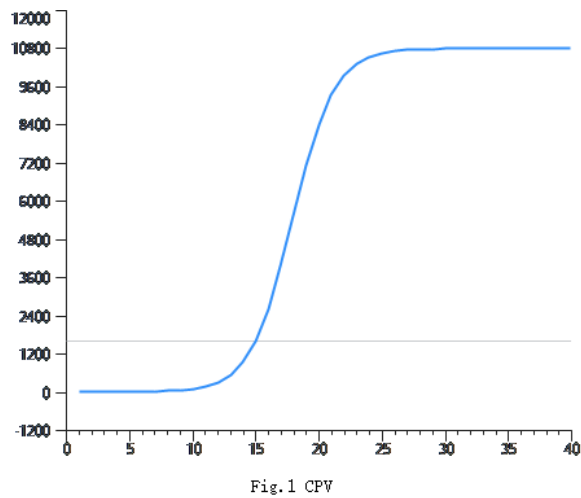

Result Interpretation:

- 1. Positive Result (+): The current test sample contains the target substance (pathogen or internal control);
 - 2. Negative Result (-): The target substance (pathogen or internal standard) in the current test sample is either below the detection limit or absent;
 - 3. CT > Ref. Range, suggests infection window or recovery phase. Clinical correlation required. Recommend retesting within 24-48 hours to monitor CT dynamics;
 - 4. CT Number Reference Interval: Reference interval used to distinguish the presence or absence of the target substance based on CT numbers.If CT > 30, the viral load is low, and the risk of transmission is low, indicating that the animal may be asymptomatic or in a subclinical state.
- Note: The test results are only valid for the samples submitted this time and are for clinical reference only.

Testing Physician: Chief Physician: Hospital Tel.: 09061211260 Report Date: 2025-10-18

Hospital Addc: SM CITY CDO UPTOWN, MASTERSONS AVE., CARMEN, CAGAYAN DE ORO

